



正 本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 **試驗報告** **土城場區**
Date: May. 01, 2017 Date of Receipt: Apr. 11, 2017 **TEST REPORT** **TUCHENG**

報告編號: TF604182 數量: IPC 報告頁次/頁數: (P1/3) 來文字號: NIL
Report No.: TF604182 Quantity: IPC Page Order/Pages: (P1/3) Ref. No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK
Report Title: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD Item: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan
Address: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

Test Items	Test Results	Test Methods
Protection Efficiency of Mask(%) (0.075 μm NaCl, CMD)	1	99.99
	2	99.98
	3	99.98
	4	99.99
	5	99.98
	6	99.98
	7	99.98
	8	99.98
	9	99.98
	10	99.99
	Ave.	99.98
		CNS 14755 Z2125-2011 Flow rate:85.2 (Liter/min)

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

附記: 1.本報告僅對樣品負責, 樣品保留期限為一個月。

Note: This report is only responsible for the subm sample(s), which will be kept for one month period

2.本報告非經本檢測及驗證部書面同意, 不得摘錄或全部複製除外。

This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3.試驗報告所載事項不得作為公開廣告及商業推銷之用。

The test report should not be used for public advertisement and commercial promotion.



財團法人紡織產業綜合研究所

長 授 權 核 發 人:

Authorized by president of Taiwan Textile Research Institute

紡織所檢測及驗證部

Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)

Tel: +886-2-22670321 ext. 7107, 7110

+886-2-22698229, +886-2-22698230

Fax: +886-2-22675108, +886-2-22689839

Gwo-Tsun Jou

Director.
Department of Testing and Certification



正本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 **試驗報告** **土城場區**
Date: May. 01, 2017 Date of Receipt: Apr. 11, 2017 TEST REPORT TUCHENG

報告編號: TF604182 數量: 1PC 報告頁次/頁數: (P2/3) 來文字號: NIL
Report No.: TF604182 Quantity: 1PC Page Order/Pages: (P2/3) Ref. No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK
Report Title: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD Item: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan
Address: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

Test Items	Test Results	Test Methods
Inhalation Resistance (Pa)	1	147.00
	2	131.32
	3	146.02
	4	135.24
	5	126.42
	6	133.28
	7	129.36
	8	121.52
	9	125.44
	10	155.82
	Ave.	135.14
Exhalation Resistance (Pa)	1	167.58
	2	146.02
	3	163.66
	4	157.78
	5	148.96
	6	153.86
	7	147.98
	8	141.12
	9	147.00
	10	177.38
	Ave	155.13

Note: 1mmH2O=9.8Pa.

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

附記: 1.本報告僅對樣品負責, 樣品保留期限為一個月。
Note: This report is only responsible for the subn- sample(s), which will be kept for one month period.
2.本報告非經本檢測及驗證部書面同意, 不得摘錄或但全部複製除外。
This report cannot be reproduced in any way, ex- full context, without the prior approval in writ- this Department of Testing and Certification.
3.試驗報告所載事項不得作為公開廣告及商業推銷。 The test report should not be used for public adverti- and commercial promotion.

財團法人紡織產業綜合研究所
長 授權核發人: *Guo-Tsun Jou*
Authorized by president of Director.
Taiwan Textile Research Institute Department of Testing and Certification
Department of Testing and Certification, Taiwan Textile Research Institute
No. 350, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
+886-2-22698229, +886-2-22698230
Fax: +886-2-22675108, +886-2-22689839



正 本
ORIGINAL

試驗報告 土城場區
TEST REPORT TUCHENG

日期: May. 01, 2017 收件日期: Apr. 11, 2017

報告編號: TF604182 數量: 報告頁次/頁數: 1 來文字號: (PI) No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan


Test Items		Test Results	Test Methods
Air Exchange Pressure (mmH2O/cm ²)	1	5.3	CNS 14777 T4039-2003
	2	4.4	
	3	5.4	
	4	5.8	
	5	4.9	

Note: Air Exchange Pressure takes 5 masks for testing.

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

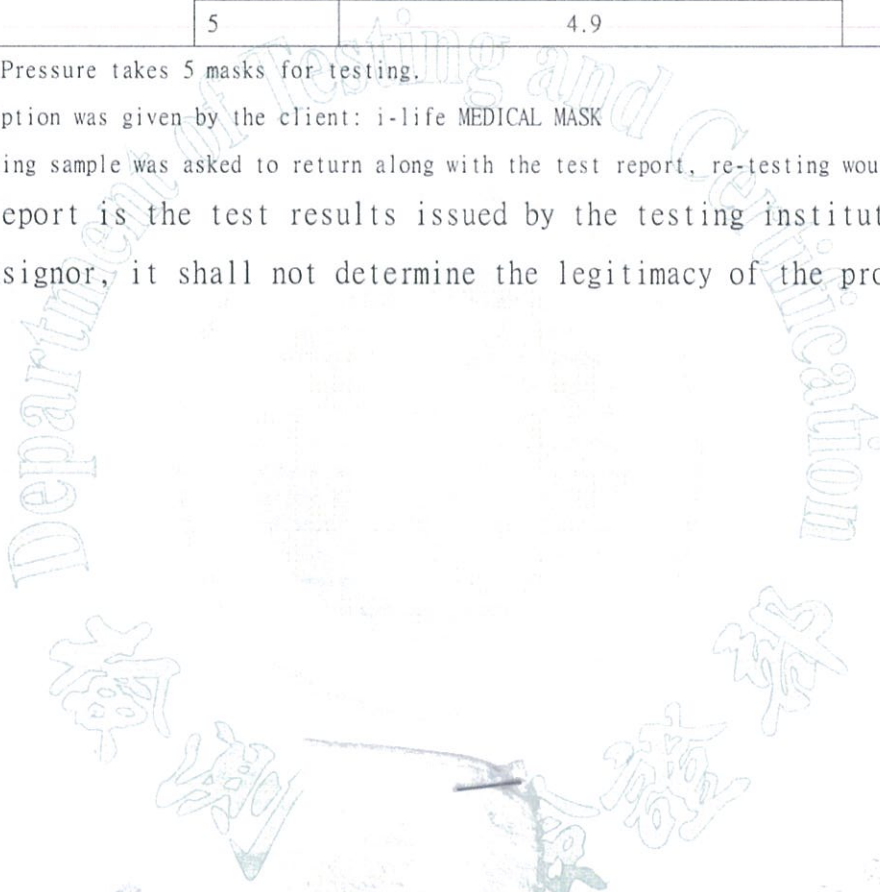

Gwo-Tsun Jou

附記: 1. 本報告僅對樣品負責, 樣品保留期限為一個月。

Note: This report is only responsible for the submitted sample(s), which will be kept for one month period.

2. 本報告非經本檢測及驗證部書面同意, 不得摘錄複製, 但全部複製除外。

This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3. 試驗報告所載事項不得作為公開廣告及商業推銷之用。

The test report should not be used for public advertisement and commercial promotion.



Director,
Department of Testing and
Certification

財團法人紡織產業綜合研究所
長授權核發人
Authorized by president of
Taiwan Textile Research Institute

財團法人紡織產業綜合研究所
檢驗及驗證部 新北市土城區承天路六號
Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
+886-2-22698229, +886-2-22698230
Fax : +886-2-22675108, +886-2-22689839