



正本  
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 試驗報告 TEST REPORT 土城場區 TUCHENG

報告編號: TF604182 數量: 1PC 報告頁次/頁數: (P3/3) 來文字號: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK


地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

Test Items		Test Results	Test Methods
Synthetic Blood Penetration Pressure: 120 mmHg	1	none	CNS 14774 T5017-2011 9.5
	2	none	CNS 14776 T4038-2003
	3	none	
	4	none	
	5	none	
	6	none	
	7	none	
	8	none	
	9	none	
	10	none	

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

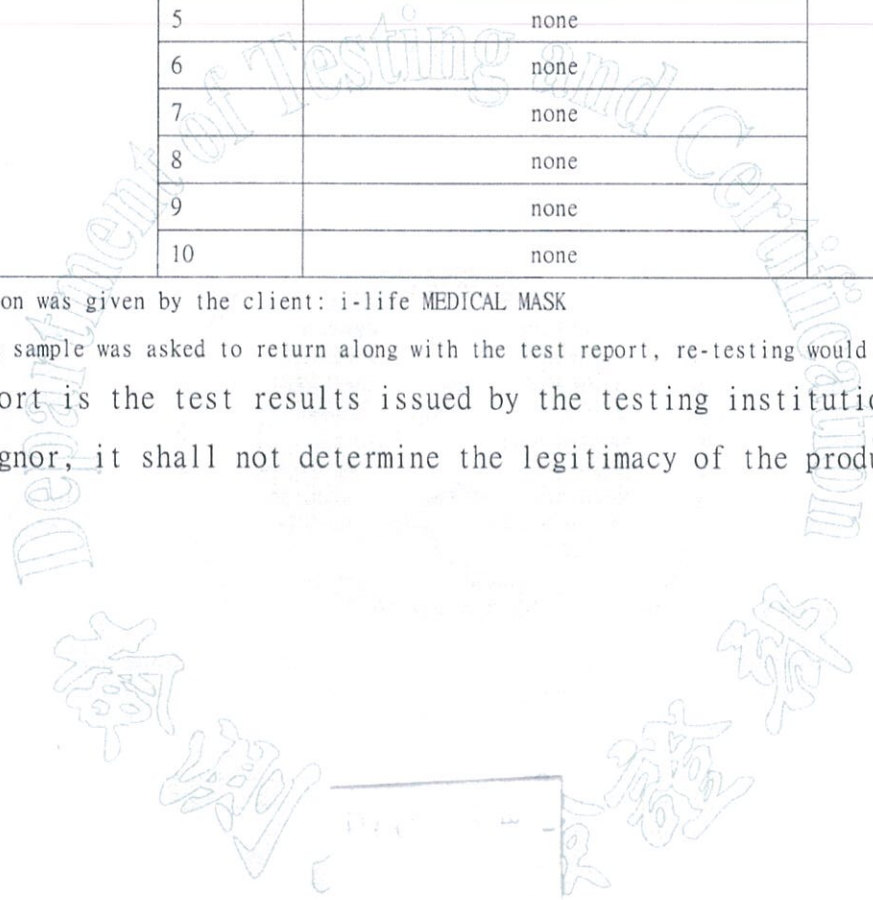

附記: 1. 本報告僅對樣品負責，樣品保留期限為一個月。  
Note: This report is only responsible for the submitted sample(s), which will be kept for one month period.  
2. 本報告非經本檢測及驗證部書面同意，不得摘錄複製但全部複製除外。  
This report cannot be reproduced in any way, except in full context, without the prior approval in writing from this Department of Testing and Certification.  
3. 試驗報告所載事項不得作為公開廣告及商業推銷之用  
The test report should not be used for public advertisement and commercial promotion.

財團法人紡織產業綜合研究所  
主任授權核發人: *Guo-Tsun Jou*  
Authorized by president of  
Department of Testing and Certification  
Taiwan Textile Research Institute  
本所檢測及驗證部 新北市土城區承天路六號  
Department of Testing and Certification, Taiwan Textile Research Institute  
Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)  
Tel: +886-2-22670321 ext. 7107, 7110  
+886-2-22698229, +886-2-22698230  
Fax: +886-2-22675108, +886-2-22689839

