



正 本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 **試驗報告** **土城場區**
Date: May. 01, 2017 Date of Receipt: Apr. 11, 2017 **TEST REPORT** **TUCHENG**

報告編號: TF604182 數量: IPC 報告頁次/頁數: (P1/3) 來文字號: NIL
Report No.: TF604182 Quantity: IPC Page Order/Pages: (P1/3) Ref. No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK
Report Title: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD Item: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan
Address: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

| Test Items | | Test Results | Test Methods |
|--|------|--------------|---|
| Protection Efficiency of Mask(%) (0.075 μm NaCl, CMD) | 1 | 99.99 | CNS 14755 Z2125-2011 Flow rate:85.2 (Liter/min) |
| | 2 | 99.98 | |
| | 3 | 99.98 | |
| | 4 | 99.99 | |
| | 5 | 99.98 | |
| | 6 | 99.98 | |
| | 7 | 99.98 | |
| | 8 | 99.98 | |
| | 9 | 99.98 | |
| | 10 | 99.99 | |
| | Ave. | 99.98 | |

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

附記: 1.本報告僅對樣品負責, 樣品保留期限為一個月。

Note: This report is only responsible for the subm sample(s), which will be kept for one month period

2.本報告非經本檢測及驗證部書面同意, 不得摘錄或全部複製除外。

This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.

3.試驗報告所載事項不得作為公開廣告及商業推銷之用。

The test report should not be used for public advertisement and commercial promotion.



財團法人紡織產業綜合研究所

長 授 權 核 發 人:

Authorized by president of
Taiwan Textile Research Institute

Director.

Department of Testing and Certification

紡織所檢測及驗證部 新北市土城區承天路六號
Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
+886-2-22698229 , +886-2-22698230
Fax : +886-2-22675108 , +886-2-22689839

Gwo-Tsun Jou



正本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 **試驗報告** **土城場區**
Date: May. 01, 2017 Date of Receipt: Apr. 11, 2017 TEST REPORT TUCHENG

報告編號: TF604182 數量: 1PC 報告頁次/頁數: (P2/3) 來文字號: NIL
Report No.: TF604182 Quantity: 1PC Page Order/Pages: (P2/3) Ref. No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK
Report Title: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD Item: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan
Address: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

| Test Items | Test Results | Test Methods |
|----------------------------|--------------|--------------|
| Inhalation Resistance (Pa) | 1 | 147.00 |
| | 2 | 131.32 |
| | 3 | 146.02 |
| | 4 | 135.24 |
| | 5 | 126.42 |
| | 6 | 133.28 |
| | 7 | 129.36 |
| | 8 | 121.52 |
| | 9 | 125.44 |
| | 10 | 155.82 |
| | Ave. | 135.14 |
| Exhalation Resistance (Pa) | 1 | 167.58 |
| | 2 | 146.02 |
| | 3 | 163.66 |
| | 4 | 157.78 |
| | 5 | 148.96 |
| | 6 | 153.86 |
| | 7 | 147.98 |
| | 8 | 141.12 |
| | 9 | 147.00 |
| | 10 | 177.38 |
| | Ave | 155.13 |

Note: 1mmH2O=9.8Pa.

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

附記: 1.本報告僅對樣品負責, 樣品保留期限為一個月。
Note: This report is only responsible for the subn- sample(s), which will be kept for one month period.
2.本報告非經本檢測及驗證部書面同意, 不得摘錄或但全部複製除外。
This report cannot be reproduced in any way, ex- full context, without the prior approval in writ- this Department of Testing and Certification.
3.試驗報告所載事項不得作為公開廣告及商業推銷。 The test report should not be used for public adverti- and commercial promotion.

財團法人紡織產業綜合研究所
長 授權核發人: 郭-True-Jou
Authorized by president of **Director.**
Taiwan Textile Research Institute **Department of Testing and Certification**
織所檢測及驗證部 新北市土城區承天路六號
Department of Testing and Certification, Taiwan Textile Research Institute
No. 6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
+886-2-22698229, +886-2-22698230
Fax: +886-2-22675108, +886-2-22689839



正本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 試驗報告 TEST REPORT 土城場區 TUCHENG

報告編號: TF604182 數量: 1PC 報告頁次/頁數: (P3/3) 來文字號: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK


地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

| Test Items | | Test Results | Test Methods |
|---|----|--------------|--------------------------|
| Synthetic Blood Penetration Pressure: 120 mmHg | 1 | none | CNS 14774 T5017-2011 9.5 |
| | 2 | none | CNS 14776 T4038-2003 |
| | 3 | none | |
| | 4 | none | |
| | 5 | none | |
| | 6 | none | |
| | 7 | none | |
| | 8 | none | |
| | 9 | none | |
| | 10 | none | |

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

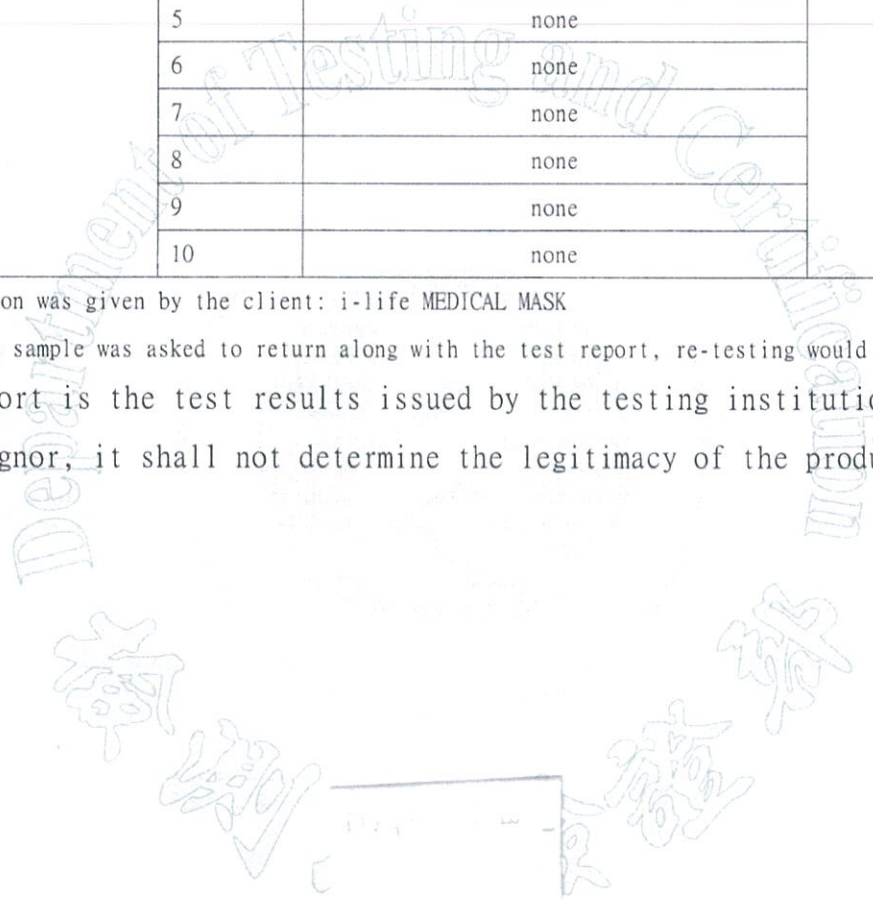

附記: 1. 本報告僅對樣品負責，樣品保留期限為一個月。
Note: This report is only responsible for the submitted sample(s), which will be kept for one month period.

2. 本報告非經本檢測及驗證部書面同意，不得摘錄複製但全部複製除外。
This report cannot be reproduced in any way, except in full context, without the prior approval in writing to this Department of Testing and Certification.

3. 試驗報告所載事項不得作為公開廣告及商業推銷之用
The test report should not be used for public advertisement and commercial promotion.

財團法人紡織產業綜合研究所
主任授權核發人: *Guo-Tsun Jou*
Authorized by president of
Department of Testing and Certification
Taiwan Textile Research Institute

本研究所檢測及驗證部 新北市土城區承天路六號
Department of Testing and Certification, Taiwan Textile Research Institute
Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)

電話: +886-2-22670321 ext. 7107, 7110
+886-2-22698229, +886-2-22698230
傳真: +886-2-22675108, +886-2-22689839





正 本
ORIGINAL

日期: May. 01, 2017 收件日期: Apr. 11, 2017 **試驗報告** **土城場區**
Date of Receipt: Apr. 11, 2017 **TEST REPORT** **TUCHENG**

報告編號: TF604182-A 數量: IPC 報告頁次/頁數: (P1/1) 來文字號: NIL
Report No.: TF604182-A Quantity: IPC Page Order/Pages: (P1/1) Ref. No.: NIL

報告抬頭: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD 試件類別: MASK
Report Title: BIOFAST BIOTECH ORIGINALITY STUDY CO., LTD Item: MASK

地址: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan
Address: No.350, Ln. 165, Sec. 1, Tanxing Rd., Tanzi Dist., Taichung City 42743, Taiwan

| Test Items | Test Results | Test Methods |
|-----------------------|--------------|--------------------------|
| Bacterial Filtration | 1 99.9 | CNS 14774 T5017-2011 9.2 |
| Efficiency (BFE)(%) | 2 > 99.9 | CNS 14775 T4037-2003 |
| Staphylococcus aureus | 3 99.9 | |
| ATCC 6538 | 4 99.9 | |
| | 5 99.9 | |

Note: Control average: 1960 CFU.

Note: Mean particle size: 3.0 μ m.


Note: Testing side: face of specimen.

Note: Testing area: 39.5 cm².

Note: Sample description was given by the client: i-life MEDICAL MASK

Note: As the remaining sample was asked to return along with the test report, re-testing would not be possible.

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

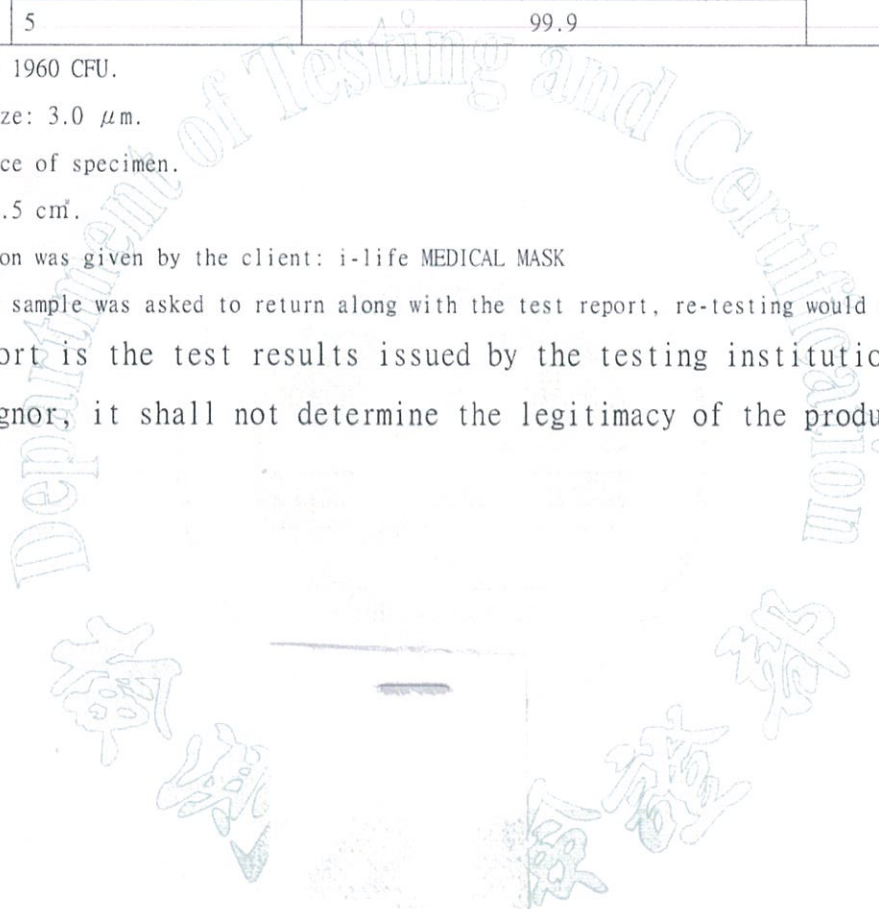

附記: 1. 本報告僅對樣品負責, 樣品保留期限為一個月
Note: This report is only responsible for the submitted sample(s), which will be kept for one month possible.
2. 本報告非經本檢測及驗證部書面同意, 不得任意複製, 但全部複製除外。
This report cannot be reproduced in any way, except in full context, without the prior approval in writing this Department of Testing and Certification.
3. 試驗報告所載事項不得作為公開廣告及商業推銷之用。
The test report should not be used for public advertisement and commercial promotion.



Gwo-Tsun Jou
財團法人紡織產業綜合研究所
所長授權核發人: _____
Authorized by president **Director.**
Taiwan Textile Research Institute **Department of Testing and Certification**
紡織所檢測及驗證部 新北市土城區承天路六號
Department of Testing and Certification, Taiwan Textile Research Institute
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R. O. C.)
Tel : +886-2-22670321 ext. 7107, 7110
+886-2-22698229 , +886-2-22698230
Fax : +886-2-22675108 , +886-2-22689839